

MANUAL tempmate.®-M1

The easy multi-use temperature datalogger



Table of content

1. Intended Use & Important Information

2

2. Disposal Instructions

2

3. Device Description & LED Indications

3

4. Equipment & Software

4

5. Quick Start Guide

4

6. Operation Instructions

5

Preparation

5

Start, Usage, Stop

5

Evaluation

7

7. FAQ

9

8. Contact Information

10

1. Intended Use & Important Information

The tempmate-M1 is an easy-to-use data logger that records all relevant temperature data during its usage. This information can then easily be read out as comprehensive and detailed PDF- or CSV-report without requiring any additional hard- or software.

The tempmate-M1 can be used for all kinds of applications where monitoring and recording temperature is required.

The data logger is provided ready-to-use in a default configuration and offers further possibilities through its free configuration software tempbase-2 (available on www.tempmate.com)

Quick Notes & Important Information:

The tempmate-M1 is a multi-use data logger; as such, it can be started and stopped without limitation.

The internal storage allows a total of 32.000 data points; once stopped and re-started, the storage will automatically be deleted.

The installed lithium battery allows a total run-time of ca. 90 days with the default configuration and if kept under optimal storage conditions (room temperatures) before; once depleted, the battery can easily be replaced.

During the activity it measures temperature between -30°C and +70°C (-22°F to 158°F) every 15 minutes.

The user can optionally configure the tempmate-M1 (through tempbase-2) before the logger was started. Start, stop, activity and status are indicated by the built-in display, which allows a fast and easy evaluation.

A full data report will be created once the data logger has been stopped and plugged in through USB. It is possible to create a temporary report while the data logger is active; while the data logger is connected, no data points are recorded.

The tempmate-M1 has no shelf-life; information on the added Validation Certificate is applicable for 2 years.

The built-in analog temperature sensor should be re-calibrated regularly / as per requirement.

2. Disposal Instructions

The tempmate-M1 has an installed CR2032 Lithium metal button cell next to electronic parts and raw materials, and therefore requires the data logger to be disposed of by a waste or recycling service provider.

3. Device Description



LED Indication

Descriptions Frontside:

- Start/Scroll Button: used to start the data logger or to scroll through different display pages
- Mark/Stop Button: used to stop the data logger or to mark an event
- USB Interface: protected by water-proof cap and used to connect to USB

Descriptions Frontside:

- Device Information: unique serial number, model number and certification
- Battery Case: can be opened to replace CR2032 lithium battery

Multi-Function Display:

The display on the frontside inform the user about every activity and status of the data logger; the status can always be requested by pushing the start or stop button once (one short click).

The display stays active for 15 seconds and shows all relevant data about the current measurement; by scrolling through the display, further information can be found.

4. Equipment & Software


The tempmate-M1 is provided ready-to-use in single units and does not need any additional hard- or software.

External sensors and mounting brackets are sold separately.

Optionally, the tempmate-M1 can be configured and evaluated through tempbase-2, which allows the user to change every setting and adapt it to their application, as well as comprehensive possibilities to archive and work with recorded data.

Tempbase-2 can be downloaded for free on www.tempmate.com

5. Quick Start Guide

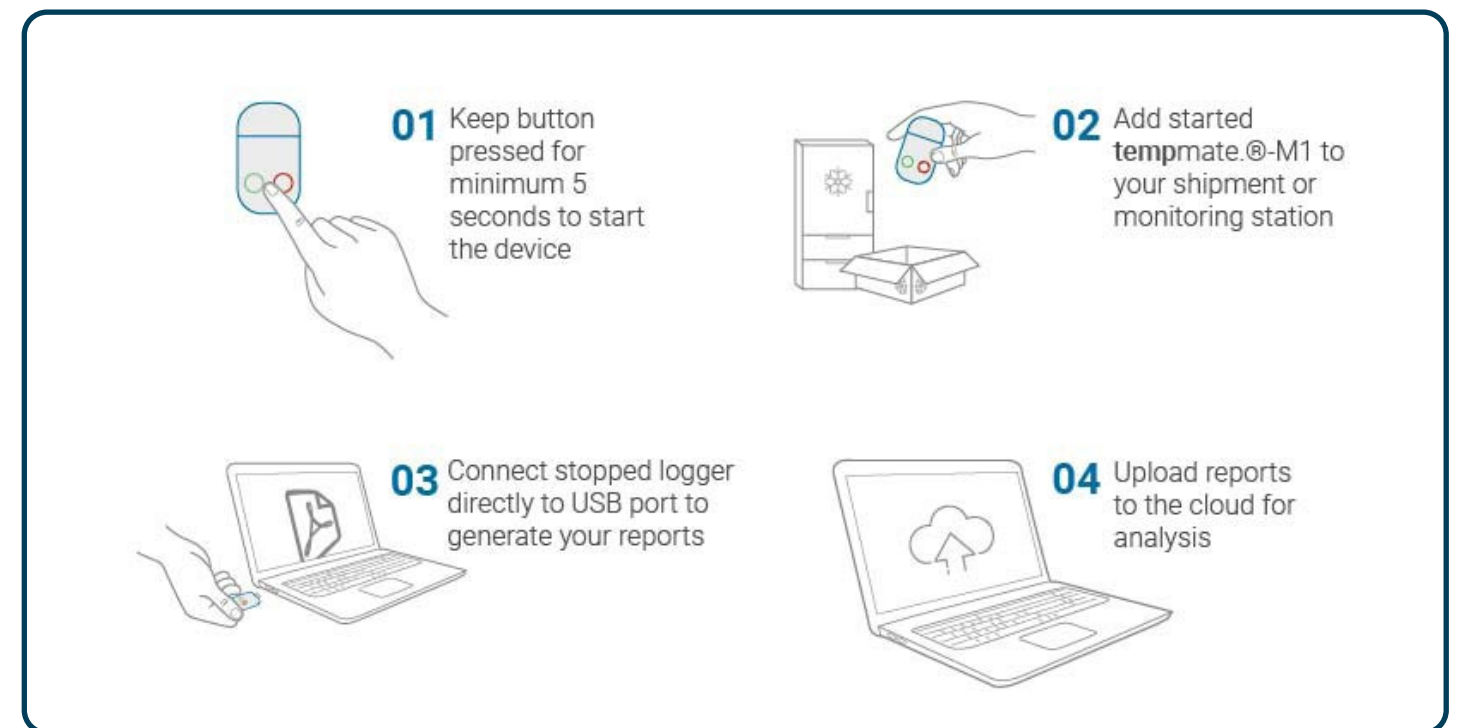

- 1.** To start, keep the Start/Scroll Button pushed for minimum 5 seconds, until the display shows "REC"
- 2.** Place the data logger and record the ambient temperature
- 3.** To stop, keep the Start/Stop Button pushed for minimum 5 seconds, until the display shows "STOP"
- 4.** Plug in the data logger via USB and receive the full report as PDF & CSV file

6. Operation Instructions

1st STEP PREPARATION

- no further preparation is necessary, as the data logger is provided ready-to-use;
- optionally, the user can configure the data logger through tempbase-2 before it is started;
- Important: the use of an external sensor must be configured through tempbase-2 first, before the data logger is started;
- the tempmate-M1 can be kept outside of room temperature conditions (~21°C / 70°F), but this can potentially have an impact on the installed battery;

We recommend keeping the data logger in room temperature and conditioning it only shortly before the usage. The battery must be replaced regularly.


2nd STEP START, USAGE, STOP

Starting the data logger

- To start the data logger, keep the left Start/Scroll Button  pushed for a minimum of 5 seconds, until the display shows "REC"



- Once started, the activated display will show a PLAY sign next to the current temperature; after 15 seconds, the display will shut down



- The data logger is now activated and will record the near ambient temperature
- If no start delay was set, the first temperature data point will be saved after the first measurement interval is due
- If a start delay was set, the first data point will be recorded after the delay is due, and then follow the set measurement interval

Usage while active

- The data logger should be placed as close as possible to the place of use; it should not be placed in-between or under heavy storages
- To fix the data logger on a surface, an optionally available mounting bracket can be used (magnetic or screwed)

Status Request:

The status can always be requested by pushing the Start/Scroll or Stop/Mark button once (one short click). The built-in display stays active for 15 seconds if no button is pushed and shows all relevant data on different pages.

- If the tempmate-M1 has not been started yet, it only shows the PLAY and STOP sign simultaneously
- Once started, the display shows a PLAY sign next to the temperature
- Once stopped, the display shows a STOP sign next to the temperature

By pushing the start/stop button repeatedly (not constantly), the user can switch to different pages:



► **Page 1:** Battery Level, Activity, eventual reached alarms, current temperature




► **Page 2:** Number of currently saved readings ("LOG")




► **Page 3:** Highest measured value ("MAX")



► **Page 4:** Lowest measured value ("MIN")



► **Page 5 - 14:** configured higher and lower alarm thresholds ("H 1" / "L 1" ...)



Pause:

It is possible to pause the active measurement temporarily; during the pause, the data logger only measures time but no temperature.

This pause phase will be reflected on the PDF/CSV-report.

To activate the pause modus:

- first activate the display
- then double-click the left Start/Scroll button
- the display will confirm the activated pause



To de-activate the pause modus:

- first activate the display
- then double-click the left Start/Scroll button
- the display will confirm the de-activated pause

**Mark event:**

Certain events during the measurement can be marked manually and are reflected on the PDF/CSV-report later. In total, 10 marks are possible.

To place a mark:

- first activate the display
- then double-click the right Stop/Mark button
- the display will confirm the placed mark

**Stopping the data logger**

- To stop the data logger, keep the Stop/Mark Button  pushed for a minimum of 5 seconds until the display shows "STOP"



- Once stopped, the display will show a STOP sign

Important:

- Recorded data will be kept until the data logger is started again
- We recommend to read-out and save the recorded data as soon as the data logger is stopped
- Deleted data cannot be restored

If the data logger was read-out through tempbase-2, all data will be kept in the user database

3rd STEP EVALUATION


Evaluation on device level

Per status request (see "Usage") the user can check if an alarm threshold has been breached or what the recorded MIN and MAX temperature was

- If an alarm threshold has been breached, the display will show a related symbol in form of two arrows above the temperature:



- By pushing the Start/Scroll Button repeatedly, the recorded MIN and MAX temperature can be found on page 3 and 4 of the display.

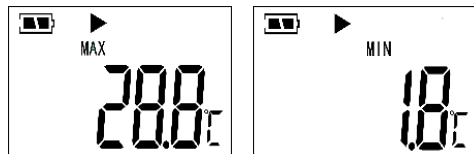

Creating PDF or CSV report


The recorded data are primarily presented as PDF report, which lists all important information about the measurement.

- Remove the protection cap and plug-in the data logger via USB
- Once plugged in, the display activates and shows "PDF"



- During this, all recorded data is processed into a readable format and depending on the number of data points, this process can take up to 2 minutes. Please do not unplug the data logger during this process!

- Once all data is processed, the display will show "USB"



- The data logger will be recognized as flash-drive and will list all available files, including the report as PDF file.
- The report(s) can be saved locally via drag & drop, or by opening the files and save them through their application (Adobe Acrobat Reader recommended)


Important:

- the PDF/CSV reports are only created momentarily; once the data logger is unplugged, they must be created again
- the files on the data logger cannot be deleted completely, and deletion is not recommended; if they were deleted by the user on the device, they could be re-created by connecting them to USB again

OTHER DISPLAY STATES



The display shows „Out d“ when the device's time and date are outdated; replace the coin battery and re-configure the logger via tempbase-2 to resolve this.




The display shows „rE-CF“ indicating that the logger requires re-configuration via tempbase-2.


Evaluation on software level

Optionally or additionally to the PDF report, the recorded data can also be loaded into tempbase-2. This gives the user the ability to see the data of plugged-in devices, export them into different formats, create an archive of already installed devices, and more.

- Plug-in data logger via USB and wait until all data is processed
- Start tempbase-2
- tempbase-2 will load all data from the installed unit into its database and will open the "Summary"
- Graph will show the temperature process as graph
- Table will show all recorded data as list

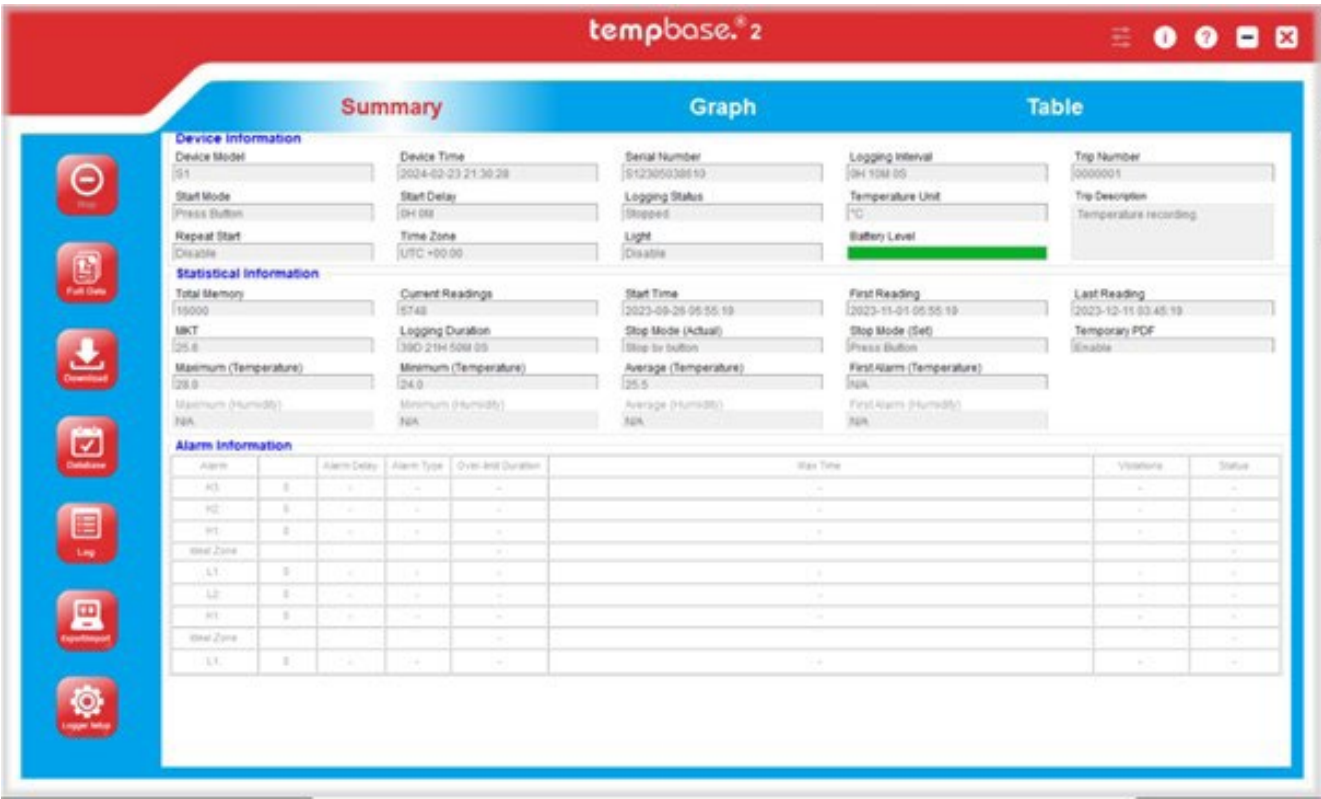

- All data can optionally be exported as PDF or XLS file

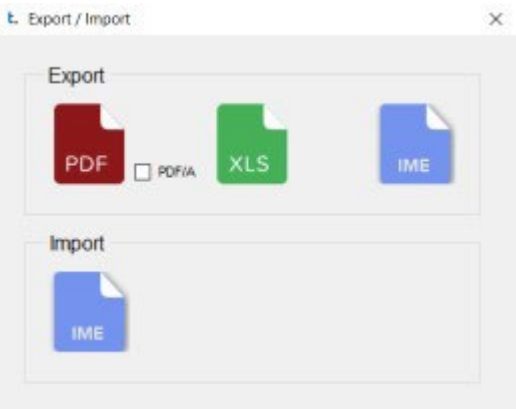


- Each data logger plugged in will automatically create an entry in the local Database and can be accessed later

[1]	Status	Data ID	Start Time	Current Readings	S1 (Max)	S1 (Min)	S2 (Max)	S2 (Min)
▶	✓	M2T231000137_20240223122917	2024-02-08 09:40:49	2171	25.9 °C	21.8 °C	N/A	N/A
✓	✓	M2T231000137_20240222150134	2024-02-08 09:40:49	2043	25.9 °C	21.8 °C	N/A	N/A
	✓	S12305038610_20240220094513	2023-09-26 05:55:19	5748	28.0 °C	24.0 °C	N/A	N/A
	✓	S12305038610_20240220093633	2023-09-26 05:55:19	5663	44.9 °C	11.2 °C	N/A	N/A
	✓	M2T231000137_20240214110349	2024-02-08 09:40:49	867	25.5 °C	22.1 °C	N/A	N/A
	✓	S2T2301029002_20240202114812	2023-12-15 12:09:23	553	9.0 °C	5.0 °C	N/A	N/A
	✓	S2T2211024310_20240202114642	2024-01-25 07:26:48	12	21.1 °C	20.9 °C	N/A	N/A
	✓	S2T2301029001_20240202114332	2023-12-15 12:09:42	553	8.4 °C	5.0 °C	N/A	N/A
	✓	S12308008120_20240131102312	2023-10-05 07:14:20	16000	25.4 °C	17.7 °C	N/A	N/A
	✓	TMM230400666_20240130113258	2024-01-02 14:14:50	8044	27.9 °C	18.7 °C	N/A	N/A
	✓	TMM230400666_20240130113242	2024-01-02 14:14:50	8044	27.9 °C	18.7 °C	N/A	N/A
	✓	TMM230400666_20240130112815	2024-01-02 14:14:50	8043	27.9 °C	18.7 °C	N/A	N/A
	✓	TMM230400666_20240130110519	2024-01-02 14:14:50	8038	27.9 °C	18.7 °C	N/A	N/A


Please refer to the tempbase-2 manual for a full description of each function

Evaluation on cloud level

To save and share the recorded data, the PDF-report can be uploaded to an existing account in the tempmate-Cloud optionally or additionally.

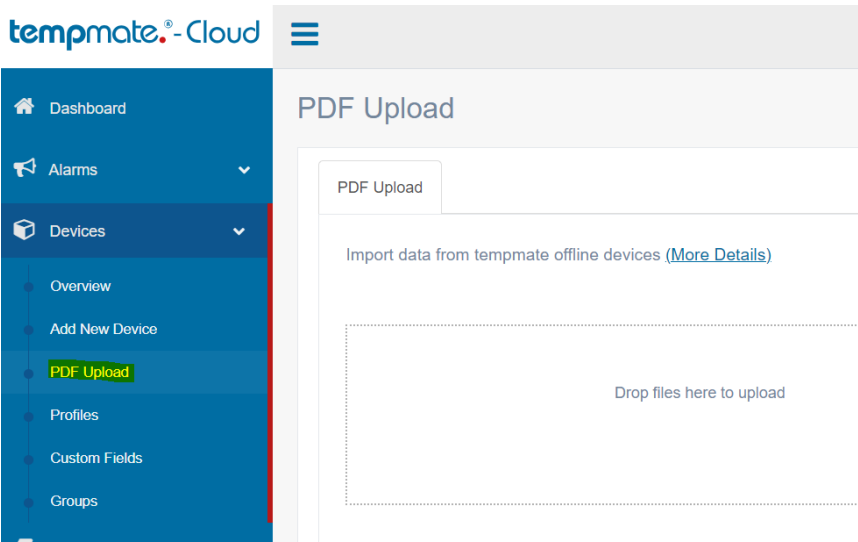

Uploaded data reports can then be found within the user's device-overview, from there they can be evaluated later or shared externally.

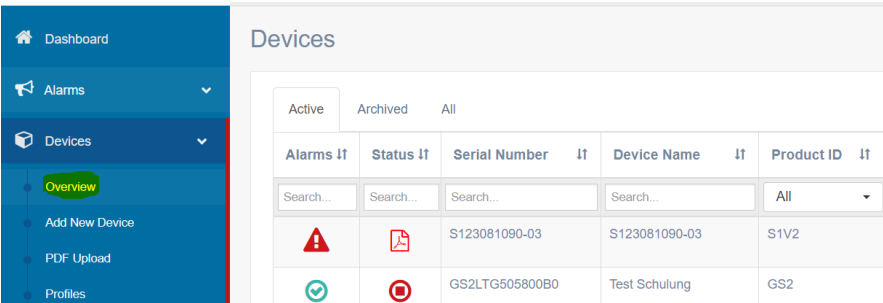

Currently it is only possible to upload PDF reports directly from the data logger, not those exported through tempbase-2!

7. FAQ – Frequently Asked Questions

Q: How often can the M1 be restarted?

A: As a multi-use device, the usage of the tempmate-M1 is not limited.

Q: How long does the battery last and when does it have to be replaced?

A: A new and fully loaded lithium coin battery allows a running time of ca. 90 days when used in room temperature conditions. Very low or very high temperatures can have a negative effect on the battery capacity and lower the running time. It is recommended to replace the battery depending on the usage, latest when the battery level on the display shows it as (almost) depleted.

Q: What happens if the data logger is not stopped?

A: The tempmate-M1 has an internal memory capacity of 32.000 data points. If this capacity is reached, the measurement stops, and no further temperature is recorded.

A "Ring Buffer" can be set up optionally through tempbase-2; with this configuration, the oldest data points will be overwritten once the memory capacity is reached.

Q: Does the M1 have an expiry date?

A: The tempmate-M1 does not have an expiry date or shelf-life.

Q: I need the calibration certificate of this data logger, where can I receive it?

A: As batch-calibrated device each data logger comes with a permanently stored validation certificate in PDF format, which informs about the calibration process during the production. The validation certificate valid for 2 years after production date.

Q: Does the M1 need to be (re-)calibrated?

A: The accuracy of the internal analog sensor should be re-calibrated regularly as per user requirement. The information about the batch-calibration on the validation certificate is valid for 2 years after production date.

Q: The PDF-report is unreadable, it shows unusual symbols.

A: The PDF-report can be re-created once the data logger was stopped. Keep the start/stop button pushed for 5 seconds, the display will show "PDF re". Once finished, the data logger can be read out again.

tempmate GmbH
Wannenäckerstr. 41
74078 Heilbronn, Germany

Tel. +49-7131-6354-0
sales@tempmate.com
www.tempmate.com

PLEASE, contact us for further questions.